
Microscope parts: label and apply

Name: _____ Class: _____ Date: _____

Compound light microscope

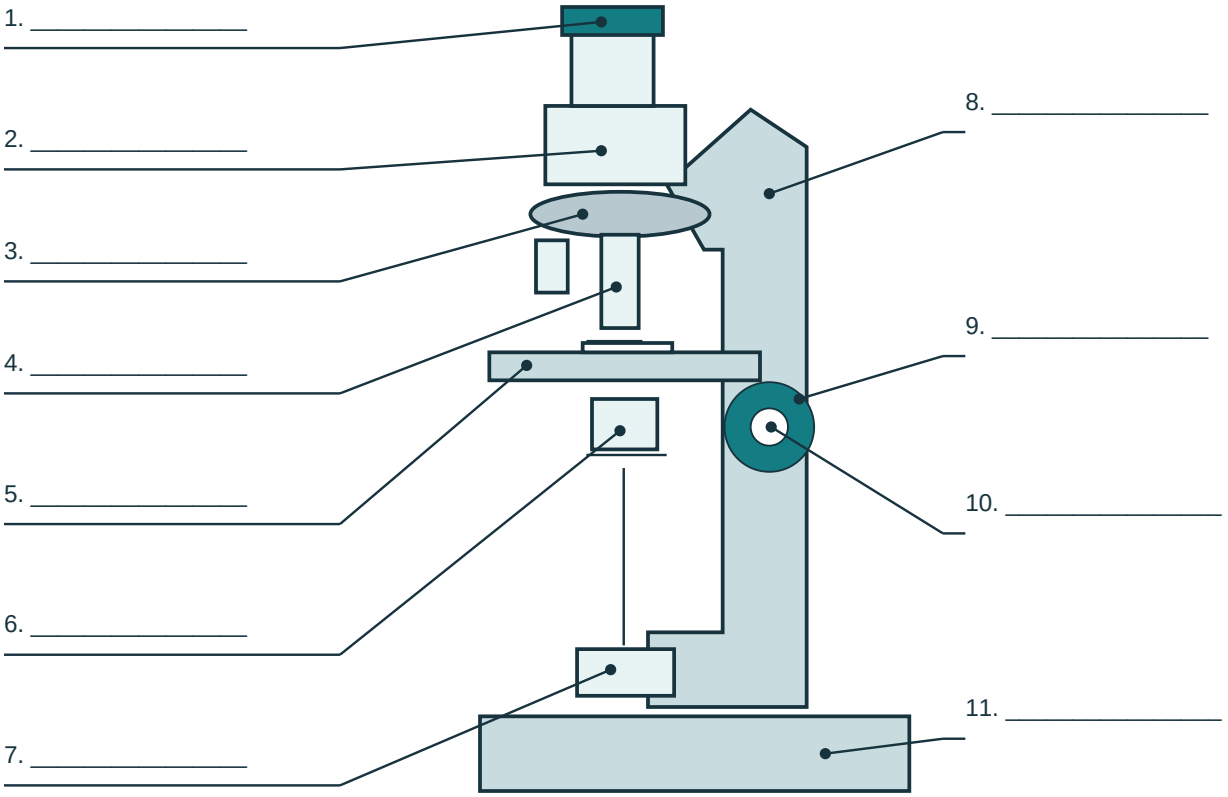

Side-view model: controls and optics differ by instrument. Stage aperture is the opening below the slide. Rack/focus stop is model-specific and is not shown. Never adjust a rack stop as a student. Use the manufacturer's instructions.

Use the reference page or your instrument manual to label 1-11.

1. With a 10x eyepiece and 4x objective, what is total magnification?

2. Which focus control should you use at high power, and why?

3. What is one safe way to carry your classroom instrument?